

# VERIFICATION OF CALIBRATION REPORT

of Datamaster cdm

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

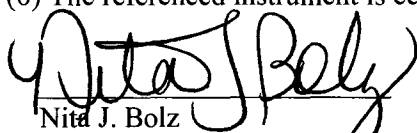
JUL 30 2009

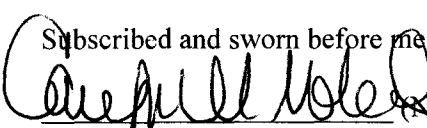
Supervisor/Operator Performing the Verification Procedure:		Datamaster cdm S/N	130309
Name		Romy Simmons	ID# 5123 Date 7/25/09
A	Agency	AST	Phone # 8323-8300
Instrument Location Mat SV West			
Alco S/N		X124658	Target Value .080 High Pressure 1200
B	Alco Test Value Average		
	1 <sup>st</sup> Alco	.081	2 <sup>nd</sup> Alco .080
Signature		RASJ	
CUB 8/6/09			
(OVER)			


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 14<sup>th</sup> day of August, 2009.  
  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of Datamaster cdm

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Datamaster cdm S/N 130309

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130309

JULY 25, 2009

OPERATOR'S NAME:

SIMMONSON, NWA

OPERATOR'S NUMBER: 5123

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI:

N

O.L. #: 0

DEPT/AGENCY: PLMO

CASE/REPORT: 0

TEST TYPE: U

ALCO TARGET VALUE: .000

ALCO B/M: 012453

--- BREATH ANALYSIS ---

.002 ADJUSTED FOR 30.07 in  
ALCO TARGET .000 00:50  
BLANK TEST .000 00:51  
INTERNAL STANDARD VERIFIED 00:51  
ALCO TO 30.07 in .001 00:52  
BLANK TEST .000 00:52  
SUBJECT SAMPLE .000 00:53  
BLANK TEST .000 00:54  
ALCO TO 30.07 in .000 00:54  
BLANK TEST .000 00:55

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130309

JULY 25, 2009

TIME 00:55

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATER:

SAMPLE CHAMBER:

BREATH TUBE:

43c

40c

BAROMETER: 30.07 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

TEST 1: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

11/11/2009 11:11:11 AM  
HICKLINOPORTSUS 11/11/2009 11:11:11 AM  
perstusvml(1) 11/11/2009 11:11:11 AM